


## Certificate of Analysis

### Product Description


|                         |                                 |
|-------------------------|---------------------------------|
| Product Name            | Lenti-III-mir-GFP Control Virus |
| Cat Number              | m002                            |
| Lot Number              | KL8150                          |
| Quantity                | 2 x 50 µl                       |
| Fluorescence Tag        | GFP                             |
| Viral Titer             | 5.36 x 10 <sup>8</sup> IU/ml    |
| QC Evaluation Cell Line | 293T Cells (Cat no. LV010)      |

### Specifications

|                     | Test Method             | Minimum                     | Results                      |
|---------------------|-------------------------|-----------------------------|------------------------------|
| Viral Titer         | qRT-PCR                 | 1.0 x 10 <sup>7</sup> IU/ml | 5.36 x 10 <sup>8</sup> IU/ml |
| Transduction Signal | Fluorescence Evaluation | ***                         | Positive                     |
| Sterility Test      | Direct Culture          | ***                         | Not detected                 |

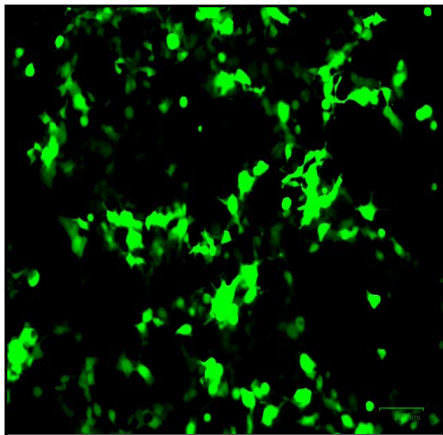

Fluorescent Tag: GFP

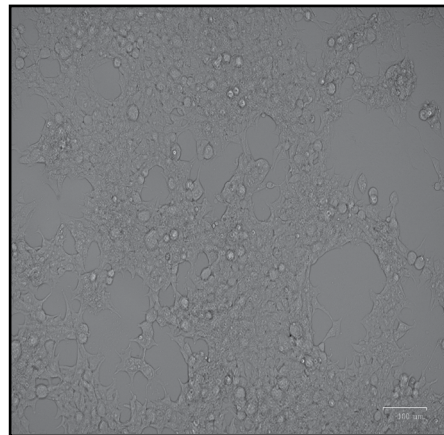

Brightfield Image

Transduction Duration: 72 Hours

MOI: 10.7

Multiplicity of Infection (MOI) Calculation Method:

$$\text{MOI} = \frac{\text{Product Titer (IU/ml)} \times \text{Virus Volume (ml)}}{\text{Total Cell Number}}$$

This product is for research use only and is not intended for therapeutic or diagnostic applications.  
Please contact a technical service representative for more information.

1-3671 Viking Way,  
Richmond, BC, Canada V6V2J5  
Tel: 604-247-2416  
Fax: 604-247-2414  
www.abmGood.com




# Lentivirus qRT-PCR Titer Report

Cat No. m002

Lenti-III-mir-GFP Control Virus

(05/10/2016)

Viral RNA was extracted from lentivirus and cDNA was generated from RT. The viral RNA samples (diluted 100 folds) and the lentiviral RNA STD1 and STD2 are subjected to qRT-PCR to determine threshold cycle (Ct) values. Real-time PCR was processed using lentivirus specific primers. With Ct values, the titers of lentivirus were determined by our lenti-titer calculator.

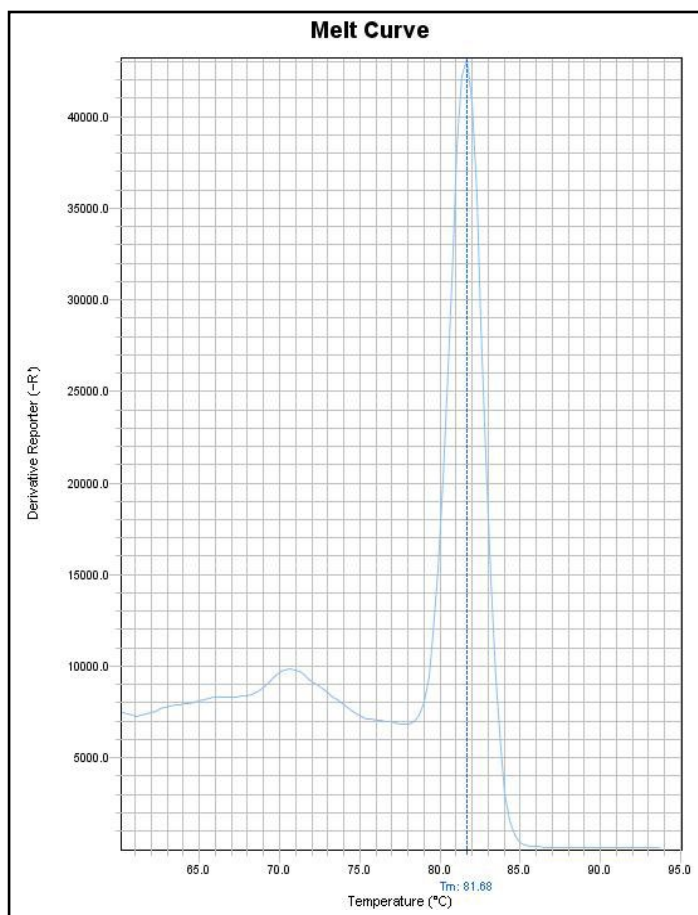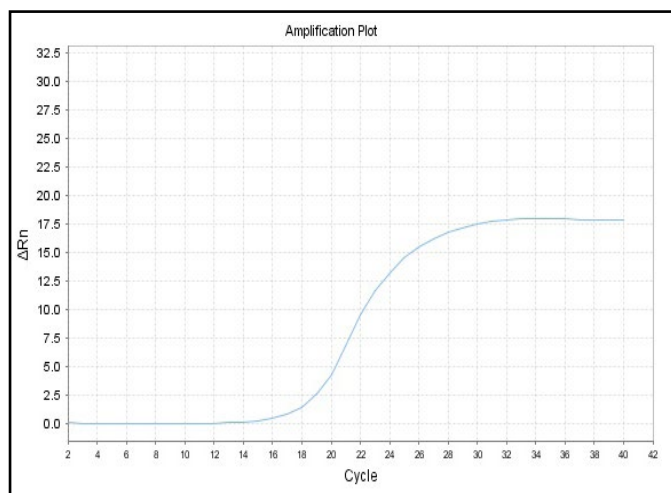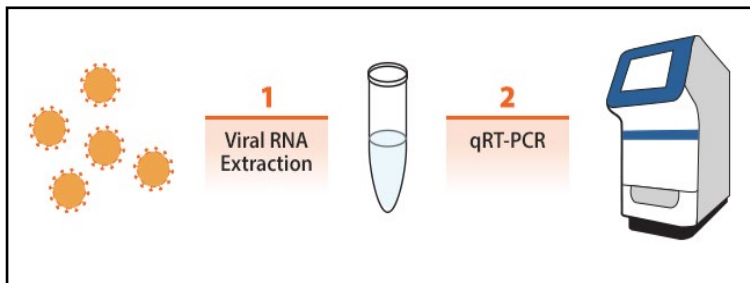

|                                |                  |
|--------------------------------|------------------|
| <b>Block Type</b>              | 48well           |
| <b>Chemistry</b>               | SYBR_GREEN       |
| <b>Experiment Run End Time</b> | 05/10/2016 13:20 |
| <b>Instrument Type</b>         | ABI Step one     |
| <b>Passive Reference</b>       | ROX              |

| Sample Name          | Lenti-III-mir-GFP Control Virus | STD1  | STD2  |
|----------------------|---------------------------------|-------|-------|
| C <sub>T</sub> Value | 18.86                           | 15.73 | 18.65 |

Titer of **Lenti-III-mir-GFP Control Virus** =

$$\left[ 5 \times 10^7 / 2^{3(C_{Tx} - C_{t1}) / (C_{t2} - C_{t1})} \right] \times 100 = 5.36 \times 10^8 \text{ IU/ml}$$

C<sub>tx</sub>: Ct value of sample, C<sub>t1</sub>: Ct value of STD1, C<sub>t2</sub>: Ct value of STD2.

(Note: the titer equation was multiplied by 100 to account for the dilution of the lentivirus sample)